SIEMENS

LITHOSTAR MODULARIS

SP

Replacement instructions

Labeling the Top Cover on the SONOCUR and LITHOSTAR MODULARIS and Vario

© Siemens AG 2000
The reproduction, transmission or use of this document or its contents is not permitted without express written authority. Offenders will be liable for damages. All rights, including rights created by patent grant or registration of a utility model or design, are reserved.

English
Print No.: SPL1-130.841.02.03.02
Doc. Gen. Date: 04.05
Replaces: SPL1-130.841.02.02.02

Chapter	Page	Revision
all	all	03

Document revision level

The document corresponds to the version/revision level effective at the time of system delivery. Revisions to hardcopy documentation are not automatically distributed.

Please contact your local Siemens office to order current revision levels.

Disclaimer

The installation and service of equipment described herein is to be performed by qualified personnel who are employed by Siemens or one of its affiliates or who are otherwise authorized by Siemens or one of its affiliates to provide such services.

Assemblers and other persons who are not employed by or otherwise directly affiliated with or authorized by Siemens or one of its affiliates are directed to contact one of the local offices of Siemens or one of its affiliates before attempting installation or service procedures.

Contents 0 - 3

Page

1 General information 1 - 1

2 SONOCUR 2 - 1

3 LITHOSTAR MODULARIS 3 - 1

4 Changes to previous version 4 - 1

NOTE

This kit contains the necessary labels for the SONOCUR and LITHOSTAR MODULARIS.
Any unused labels should be destroyed.

- In order to ensure that the same cover colors are used, always replace both halves of the covers simultaneously.
- Contents of label kit 47 83 200.

Label	Quantity	SONOCUR	LITHOSTAR MODULARIS/ Vario
Company label "SIEMENS"	2	on the right and left cover	on the right and left cover
Product name "SONOCUR Plus C"	2	on the right and left cover (for SONOCUR systems with serial number 01100 to 04999)	----------
Product name "SONOCUR Basic"	2	on the right and left cover (for SONOCUR systems with serial number 05000 and higher)	----------
Product name LITHOSTAR...	2	----------	on the right and left cover
"Caution" sign	1	beside the mains switch	beside the mains switch

This page intentionally left blank.

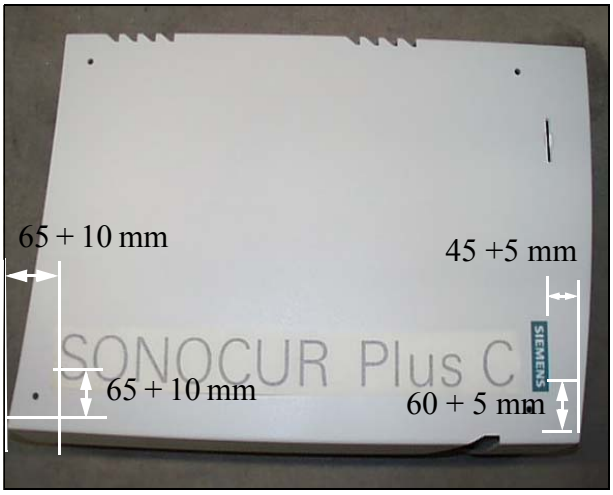

Fig. 1

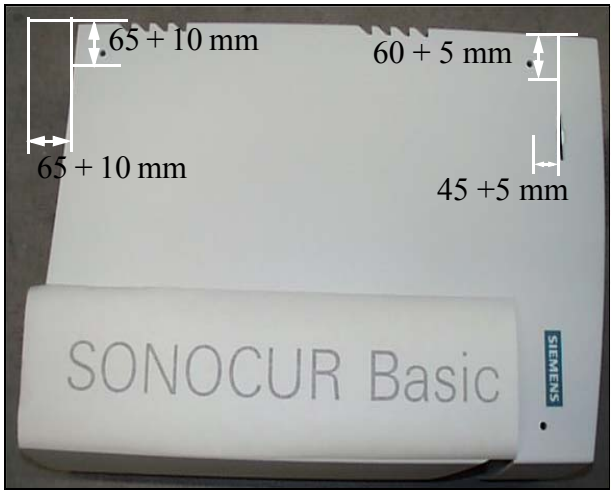

Fig. 2

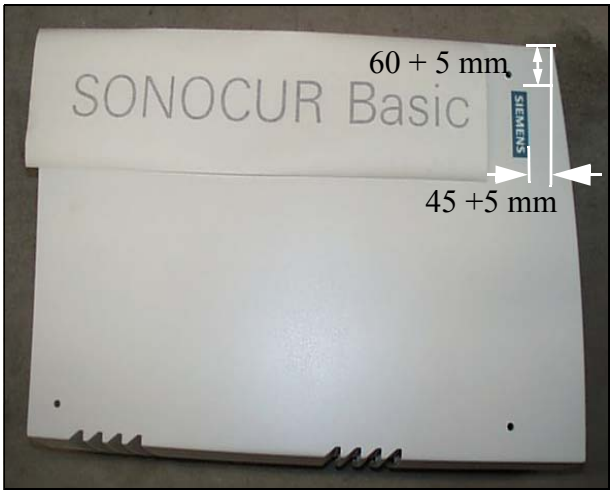

Fig. 3

Fig. 4

NOTE

The label positions described here could be different from the current position. Labels should be affixed as outlined in these instructions.

Product name "SONOCUR Plus C"	2 labels	on the right and and left covers (For SONOCUR systems with serial number 01100 to 04999)
Product name "SONOCUR Basic"	2 labels	on the right and left covers (For SONOCUR systems with serial number 05000 and higher)

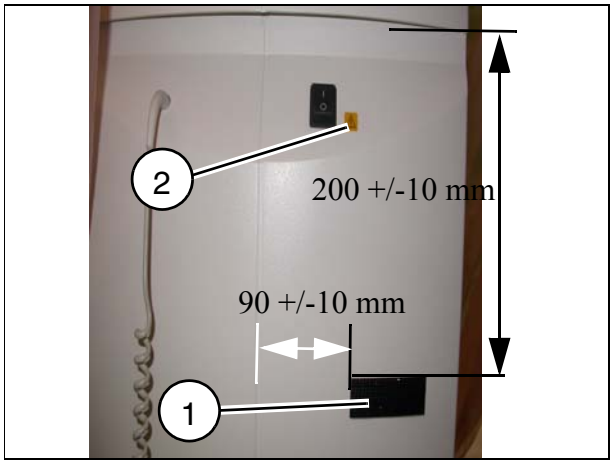

Fig. 5

- Affix the product name label on the right and left covers.
  - Remove the safety envelope.
  - Place the transparent sheet for "SONOCUR Plus" on the covers as shown in Figure 1 and Figure 2.
    Transfer the letters to the covers by rubbing.
    With the "SONOCUR Plus C" the "C" should only be transferred if "pay per use" is available.
  - Place the transparent sheet for "SONOCUR Basic" on the covers as shown in Figure 3 and Figure 4.
    (Attach the sheet at the edge of the covers).
    Transfer the letters to the covers by rubbing.
- Affix the company label on the right and left covers as shown in Figure 1 / 2 / 3 / 4.
- Affix the labels (2/ Fig.5) beside the mains switch.
- Attach the velcro closure (1/Fig. 5).
  (Several velcro closures were supplied with the first delivery. If these were not received, spare part - 15 90 822; 8 cm must be ordered).

37.5 mm - oblique measurement

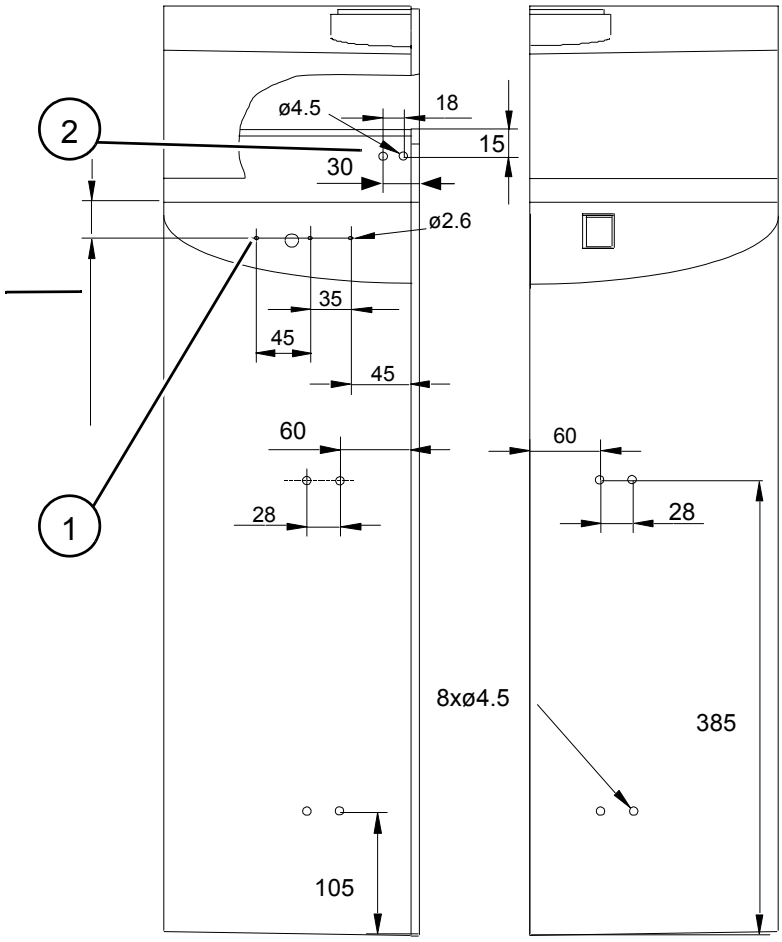

Fig. 1

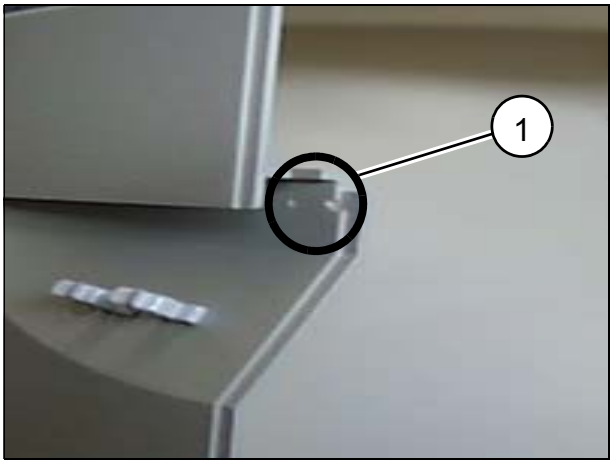

Fig. 2

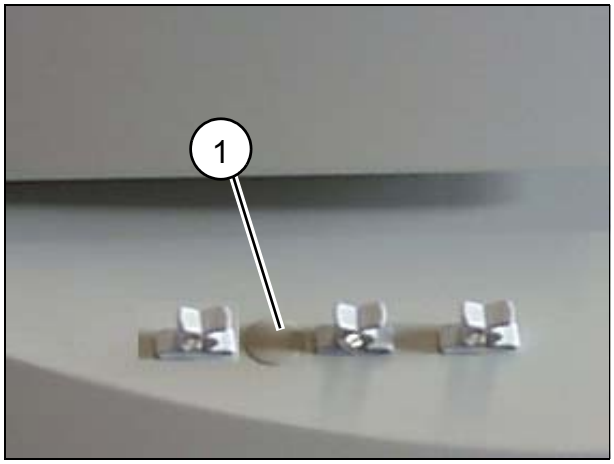

Fig. 3

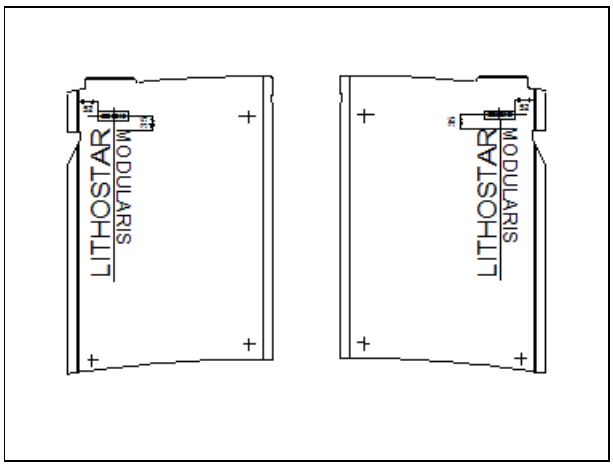

Fig. 4

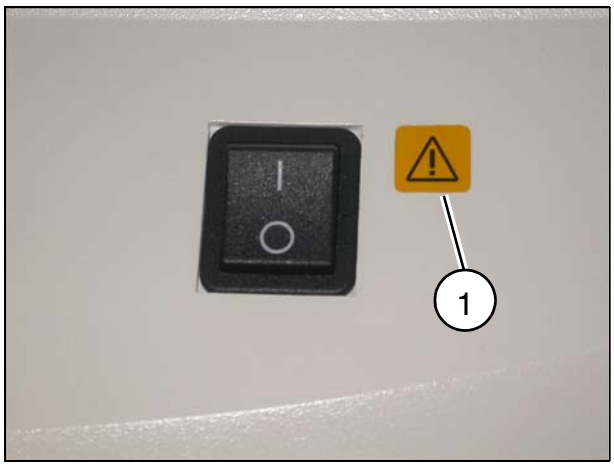

Fig. 5

- Drill the two cover halves as shown in Figure 1.
  - Pay attention to drilling the holes (2/Fig. 1); (1/Fig. 2).
  - The drilling (1/Fig. 1) should only be attached if the ultrasound option is available.
- Remove all parts of the old covers and attach them to the new covers.
- Remove the steel cover (1/Fig. 3) from the old covers and attach to the new covers.
- Affix the product name label to the right and left cover.
  - Remove the safety envelope.
  - Place the transparent sheet on the covers.
    (Attach the sheet at the edge of the covers).
  - Transfer the letters to the covers by rubbing.
- Affix the company label on the right and left cover as shown in Figure 4.
- Affix the label (1/ Fig. 5) beside the mains switch.

Chap. 0	Front page, Rev. Level and Index new generated
Chap. 2 - 2	Fig. 5 new inserted
Chap. 3 - 2	Fig. 5 new inserted

This page intentionally left blank.